



Lumbar Interbody Fusion System

Bi-Directional Expansion | Minimal Insertion Profile | Maximum Graft Delivery



INTEGRITY
IMPLANTS

OVERVIEW

FlareHawk9 is a bi-directionally expandable lumbar fusion device, featuring Adaptive Geometry™, that can be inserted at a low profile of 7mm tall by 9mm wide before expanding up to 14mm tall and to 14mm wide. With FlareHawk9, advantages formerly exclusive to either expandable or monolithic devices are united for the first time.


MINIMAL INSERTION PROFILE

Designed to minimize neural retraction during implant insertion.




BI-DIRECTIONAL EXPANSION

Stent-like technology delivers an increase in width, height, and lordosis, which is intended to resist subsidence and restore disc space height.

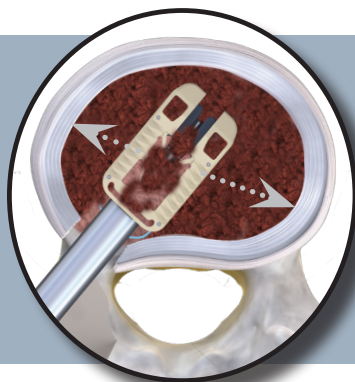


MAXIMUM GRAFT DELIVERY

The open architecture allows for continuous graft delivery through the implant and out into the disc space. Graft volume is only restricted by the quantity of disc removed.

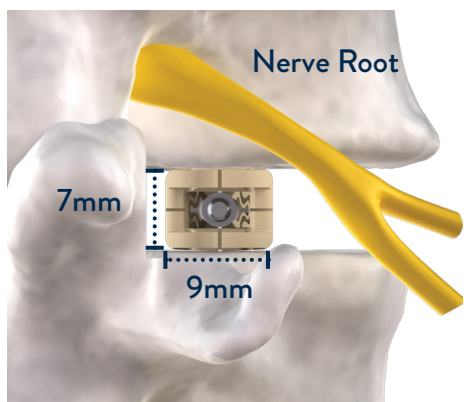

Insertion Profile

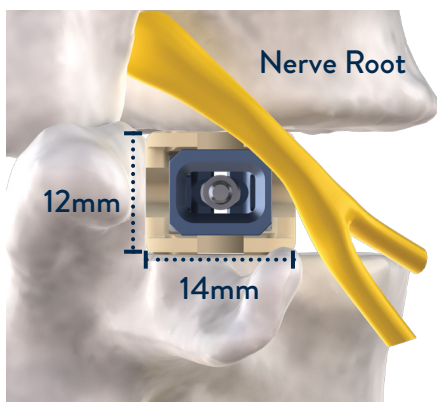

Expanded Profile



IMPLANT OFFERINGS

Lengths: 25mm & 29mm

Lordosis: 0°, 6°, 9°, & 15°

Height: 8mm to 14mm

Insertion Profile (H x W):

7 x 9mm & 9 x 9mm

Width: Starting at 9mm,
expanding to 14mm



Bi-Directional Expansion | Minimal Insertion Profile | Maximum Graft Delivery



INDICATIONS

The FlareHawk® Interbody Fusion System is indicated for spinal intervertebral body fusion with autogenous bone graft and/or allogeneic bone graft composed of cancellous and/or corticocancellous bone in skeletally mature individuals with degenerative disc disease (DDD) at one or two contiguous levels from L2 to S1, following discectomy. DDD is defined as discogenic back pain with degeneration of the disc confirmed by history and radiographic studies. These patients should have at least six (6) months of non-operative treatment. Additionally, these patients may have up to Grade 1 spondylolisthesis or retrolisthesis at the involved level(s). FlareHawk® system spacers are intended to be used with supplemental fixation instrumentation, which has been cleared for use in the lumbar spine.



Scan for FlareHawk
Animation

Refer to the FlareHawk Interbody Fusion System Instructions-for-Use (IFU) for complete contraindications, warnings, and precautions.



Integrity Implants Inc.

354 Hiatt Drive, Palm Beach Gardens, FL 33418 USA

Phone: 800 201 9300 or +1 561 529 3861

Email: customerservice@integrityimplants.com



**INTEGRITY
IMPLANTS**

integrityimplants.com
SS-00004 RevC